


# Filtration – sterile connector

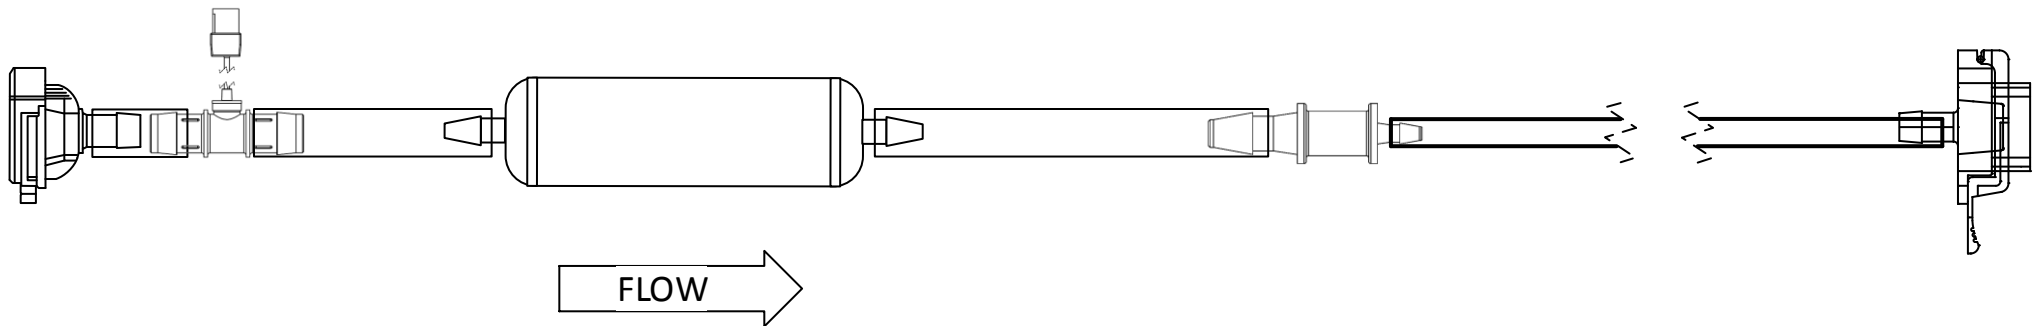

## CUSTOMER APPROVAL READ & APPROVED:

Name: \_\_\_\_\_

Date: \_\_/\_\_/\_\_

Signature: \_\_\_\_\_

## Info on Packaging & Gamma Irradiation

Packaging: double bagged  
Label: on outside bag  
Gamma Irradiation: Yes, 25-40kGy

## Bill of Materials

All connections, unless otherwise specified, are reinforced with single cable ties