


TFF tubing Retentate line
With: Bioclamp, pressure sensor, valve

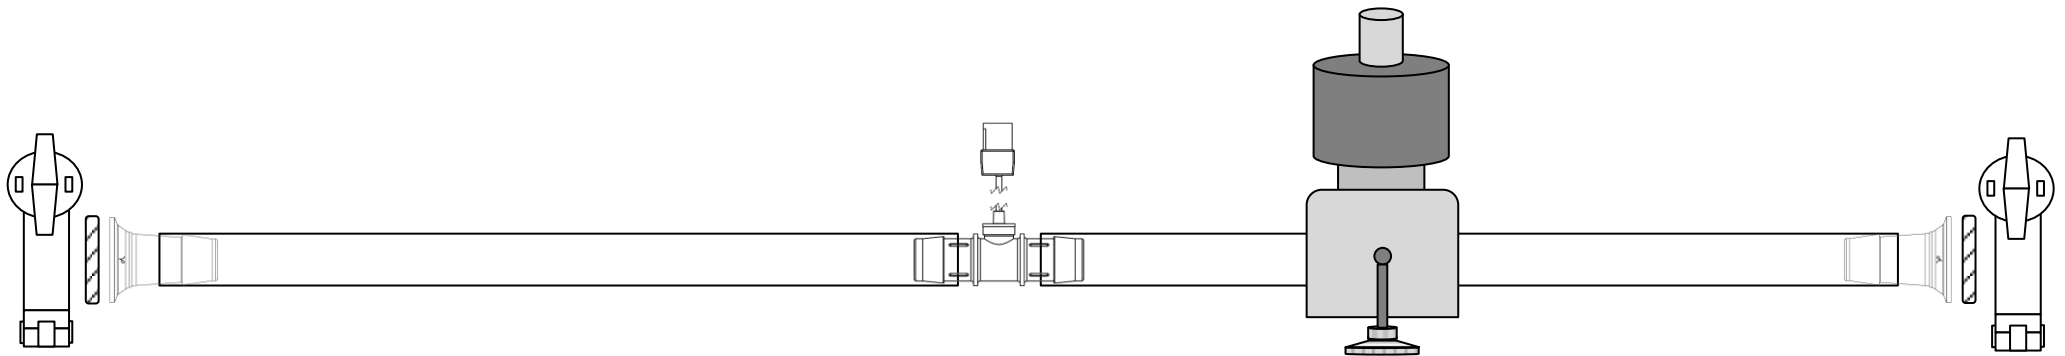

**CUSTOMER APPROVAL
READ & APPROVED:**

Name: _____

Date: __/__/__

Signature: _____

**Info on Packaging & Gamma
Irradiation**

Packaging: double bagged
Label: on outside bag
Gamma Irradiation: Yes, 25-40kGy

Bill of Materials

All connections, unless otherwise specified, are reinforced with single cable ties